

**CURRENT POSITION ID: 101DR-PT0002**

**CURRENT POSITION**

Position Name: Dryer pressure to controller  
 Location: 0025 Room  
 Plant Structure: Beamex Pharmaceutical Plant/Plant 1, Finland ( BPF )/Block 1/101 DR (Dryer 1)/

**CURRENT DEVICE**


Device ID: PT0005  
 Serial Number: 54.618  
 Manufacturer Model: Fisher-Rosemount 3051

**CURRENT PROCEDURE**

Interval: 12 months  
 Reject if Error >: 0,50 % of span  
 Adjust To <: 0,40 % of span

**CURRENT FUNCTION**

Function: Pressure Transmitter (pt)  
 Transfer Function: Linear  
 Range (I/O): 0,00 to 10,00 bar (G) 4,00 to 20,00 mA

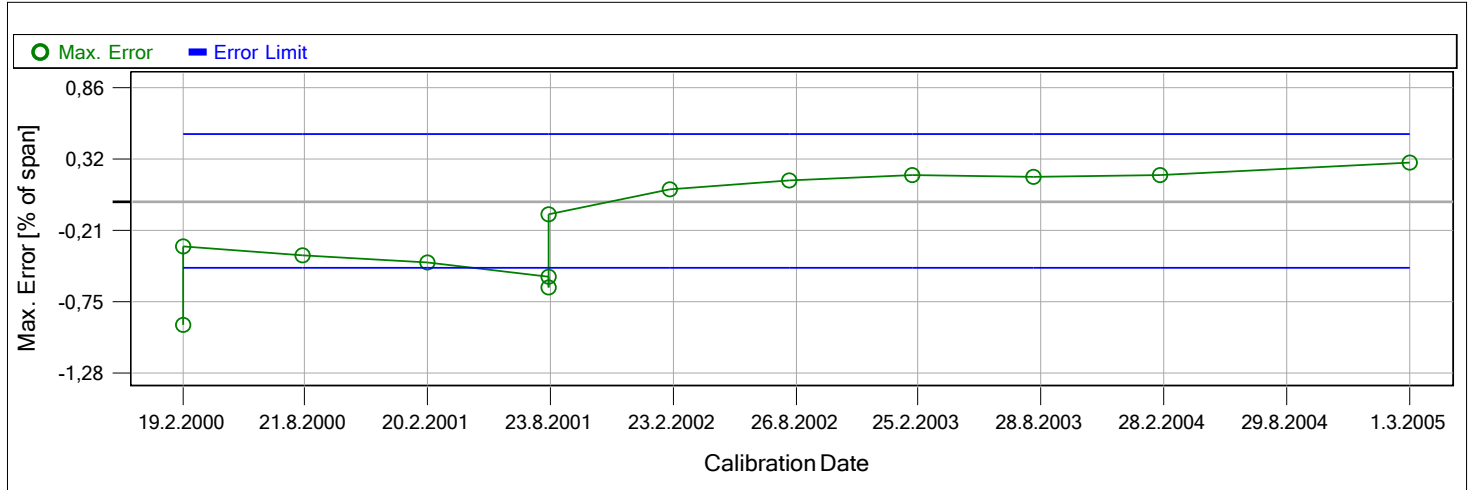

Position ID	Device ID	Serial Number	Manufacturer	Model	Calibration Date	As Found As Left	Reject if Error > [% of span]	Max. Error [% of span]	Passed Failed
101DR-PT0002	PT0002	94876	Fisher-Rosemount	3051	19.2.2000	As Found	0,5	-0,928	Failed
101DR-PT0002	PT0002	94876	Fisher-Rosemount	3051	19.2.2000	As Left	0,5	-0,340	Passed
101DR-PT0002	PT0002	94876	Fisher-Rosemount	3051	16.8.2000	As Found	0,5	-0,402	Passed
101DR-PT0002	PT0002	94876	Fisher-Rosemount	3051	19.2.2001	As Found	0,5	-0,465	Passed
101DR-PT0002	PT0002	94876	Fisher-Rosemount	3051	20.8.2001	As Found	0,5	-0,570	Failed
101DR-PT0002	PT0002	94876	Fisher-Rosemount	3051	20.8.2001	As Left	0,5	-0,643	Failed
101DR-PT0002	PT0005	54.618	Fisher-Rosemount	3051	20.8.2001	As Found	0,5	-0,095	Passed
101DR-PT0002	PT0005	54.618	Fisher-Rosemount	3051	19.2.2002	As Found	0,5	0,085	Passed
101DR-PT0002	PT0005	54.618	Fisher-Rosemount	3051	15.8.2002	As Found	0,5	0,150	Passed
101DR-PT0002	PT0005	54.618	Fisher-Rosemount	3051	17.2.2003	As Found	0,5	0,195	Passed
101DR-PT0002	PT0005	54.618	Fisher-Rosemount	3051	17.8.2003	As Found	0,5	0,188	Passed
101DR-PT0002	PT0005	54.618	Fisher-Rosemount	3051	23.2.2004	As Found	0,5	0,200	Passed
101DR-PT0002	PT0005	54.618	Fisher-Rosemount	3051	1.3.2005	As Found	0,5	0,285	Passed